

# **An International Study of Guarded Hot Plate Laboratories Using Fibrous Glass and Expanded Polystyrene Reference Materials**

By

Robert R. Zarr

Heat Transfer and Alternative Energy Systems Group  
Building and Fire Research Laboratory  
National Institute of Standards and Technology  
Gaithersburg, MD 20899-8632

And

James J. Filliben  
Statistical Engineering Division  
National Institute of Standards and Technology  
Gaithersburg, MD 20899-8980

Reprinted from STP 1426, ASTM International Standards,  
Insulation Materials, Testing and Applications, V4, 2002  
ISBN 0-8031-2898-3

NOTE: This paper is a contribution of the National Institute of Standards  
And Technology and is not subject to Copyright.

Robert R. Zarr<sup>1</sup> and James J. Filliben<sup>1</sup>

**An International Study of Guarded Hot Plate Laboratories Using Fibrous Glass and Expanded Polystyrene Reference Materials**

---

Reference: Zarr, R. R. and Filliben, J. J., **"An International Study of Guarded Hot Plate Laboratories Using Fibrous Glass and Expanded Polystyrene Reference Materials,"** *Insulation Materials: Testing and Applications: 4<sup>th</sup> Volume, ASTM STP 1426*, A. O. Desjarlais and R. R. Zarr, Eds., ASTM International, West Conshohocken, PA, 2002.

Abstract: Thermal conductivity measurements of four thermal insulation reference materials **are** presented. The measurements were obtained from an international study of guarded-hot-plate laboratories in Canada, France, Japan, the United Kingdom, and the United States. For each reference material, the study requires five independent replicate measurements at a fixed temperature of 297.15 K, **and** single-point measurements at 280 K, 290 K, 300 K, 310 K, and 320 K. **An** important finding from the replicate analysis is the existence of a laboratory-material interaction; that is, there **are** laboratory-to-laboratory differences in both location and variation that change from material to material. The major underlying source for the variability (~~both within~~ and between-laboratory) in the replicate data is discussed. The analysis of the multi-temperature (280 K to 320 K) data supports the laboratory-material interaction **as** exhibited in the fixed-temperature replicate **data**. The multi-temperature analysis also reveals an increasing difference between laboratories as the temperature departs from 297.15 K.

Keywords: certified reference material, guarded hot plate, interlaboratory, reference materials, thermal insulation, thermal conductivity, SRM

## Introduction

In 1996, an ASTM C-16 Workshop on thermal insulation Standard Reference Materials (SRMs) identified concerns with the transference of national reference materials **across** international borders [1]. Responding to similar concerns in Europe, the National Physical Laboratory began to organize an international study of guarded-hot-plate apparatus in national **standards** laboratories in Canada, France, Japan, United Kingdom, and United States in 1997. The purpose of the study was to assess the measurement variability among test results of five laboratory participants: the National

---

<sup>1</sup> Mechanical Engineer and Mathematical Statistician, respectively, National Institute of Standards and Technology, 100 Bureau Drive, Gaithersburg, MD, 20899-8632.

Research Council Canada (NRCC), Laboratoire National d'Essais (LNE), Japan Testing Center for Construction Materials (JTCCM), the National Physical Laboratory (NPL), and the National Institute of Standards and Technology (NIST). The study investigated one regional and three national reference materials. Ten specimens of each material were distributed to the participants by an issuing organization (or delegate laboratory).

This study requested two sets of data: 1) five replicate measurements of each specimen at 297.15 K (24 °C); and 2) individual (single-point) measurements at 280 K, 290 K, 300 K, 310 K, and 320 K. The test results were conducted in accordance with either International Standard Thermal Insulation–Determination of Steady-State Areal Thermal Resistance and Related Properties–Guarded Hot Plate Apparatus Test Method (ISO 8302) or ASTM Test Method for Steady-State Heat Flux Measurements and Thermal Transmission Properties by Means of the Guarded Hot Plate Apparatus, (C 177). A detailed analysis of the resulting data has been provided to the laboratory participants [2] and a summary of the results has been recently presented [3]. The present paper focuses primarily on the replicate thermal conductivity data at 297.15 K (24 °C).

### Reference Materials

The reference materials were selected to test a wide – yet manageable – variety of insulation materials from Asia, Europe, and North America. Table 1 summarizes the reference materials by designation, description, density ( $\rho$ ), thickness ( $L$ ), temperature range ( $T$ ), source, and reference. Materials 1 through 3 were fibrous in composition, ranging from 13 kg/m<sup>3</sup> to 200 kg/m<sup>3</sup>. Material 4 was a molded-beads, expanded polystyrene board (38 kg/m<sup>3</sup>). Material 3, which is a *mixture* of glass and mineral oxides fibers having high-temperature capabilities, is currently undergoing an internal review process for certification. Each issuing laboratory was responsible for characterizing and distributing 10 specimens of the reference material to the laboratory participants [2]. The European Commission Institute for Reference Materials and Measurements (IRMM) agreed to provide specimens of Certified Reference Material IRMM-440 to NPL for characterization and distribution to the participants. As a side note, the NIST Standard Reference Material Program has officially designated SRM 1451 as obsolete due to historically low customer demand. (Although obsolete, SRM 1451 is available from the Building and Fire Research Laboratory at MST.) Comparisons of the test results with predicted values of the NIST Standard Reference Materials have been presented previously [2,3].

Table 1 – *Reference Materials*

ID	Designation	Description	$\rho$ (kg/m <sup>3</sup> )	$L$ (mm)	$T$ (K)	Source and Reference
1	SRM 1451	Fibrous glass blanket	13	25	100 to 330	NIST [4]
2	IRMM-440	Resin-bonded glass fibre board	70	35	263 to 323	IRMM [5]
3	JTCCM candidate	Mineral-oxide fiberboard	200	25	---	JTCCM
4	SRM 1453	Expanded polystyrene board	38	13	285 to 310	NIST [6]

### Laboratory Apparatus

Table 2 summarizes the major parameters of the guarded-hot-plate apparatus used in this **study**. Each laboratory determined values for their relative expanded uncertainty ( $U$ ), **independently** of this study, based on international guidelines [7]. The relative expanded uncertainties reported here for a coverage factor of  $k = 2$  represent a level of confidence of approximately 95% [7]. The expanded uncertainty defines an interval about the result of a measurement that may be expected to encompass a large fraction **of** the distribution of values that could reasonably be attributed to the measurand ( $h$ ).

Table 2 – *Laboratory Guarded-Hot-Plate Apparatus*

Parameter	JTCCM	LNE	NIST	NPL	NRCC
ID	1	2	3	4	5
Plate, mm	300x300	610x610	1016 $\phi$	610x610	610x610
Meter plate, mm	150x150	300x300	406.4 $\phi$	305.2x305.2	250x250
Plate emittance	0.9	0.86 $\pm$ 0.05	0.89	>0.9	0.89
Edge guarding	Condition air	1	Condition air	2	Glass-fiber
Type of heater	Distributed	Distributed	Line source	Distributed	Distributed
Temperature sensor	Type T	Type K	PRT <sup>3</sup>	Type E	Type T
Operation mode	2-sided	2-sided	2-sided	1-sided	2-sided
$U$ ( $k=2$ ) (%)	Not reported	1.5	1.5 (IRMM-440) 1.0 (others)	1.2	1.0

<sup>1</sup>Edge insulation, temperature controlled peripheral *guard* and additional outer edge insulation

<sup>2</sup>Linear temperature gradient edge guard and 100 mm expanded polystyrene

<sup>3</sup>Platinum resistance thermometer

### Test Protocol

Under steady-state conditions, measurements of thermal conductivity<sup>2</sup> ( $h$ ) for the pair of specimens are determined using the following equation:

$$Q = \lambda 2A \frac{\Delta T}{L} \quad (1)$$

where  $Q$  is the heat flow (W) **through** the meter **area** of the specimens;  $2A$  is the meter area normal to direction of heat flow (m<sup>2</sup>);  $\Delta T$  (K) is the temperature difference across the specimen hot ( $T_h$ ) and cold surfaces ( $T_c$ ); and,  $L$  (m) is the in-situ thickness of the pair of specimens. Values of  $h$  are reported at the mean temperature,  $T_m = (T_h + T_c)/2$ .

For a single-sided mode of operation (Table 2), a single specimen is placed between the hot and cold plates of the apparatus. The other specimen is replaced with an auxiliary piece of insulation. The auxiliary *guard* plate is maintained at the same temperature as

<sup>2</sup> The thermal transmission properties of heat insulation determined from standard test methods typically include several mechanisms **of** heat transfer, including conduction, radiation, and possibly convection. For that reason, some experimentalists will include the adjective “apparent” when describing thermal conductivity of thermal insulation. However, for brevity, the term thermal conductivity will be used in this paper.

the hot plate. For determining  $\lambda$  in the single-sided case, Eq 2 is modified slightly by taking a meter area ( $A$ ) coefficient of unity.

Each participant was requested to conduct five replicate measurements for each pair of specimens at 297.15 K (24 °C) and a temperature difference of 20 K (100 observations). The operator was requested to remove the specimens from the apparatus after each measurement and re-install the specimens after sufficient conditioning. After completion of the replicate measurements, thermal conductivity measurements were conducted for each material at 280 K, 290 K, 300 K, 310 K, and 320 K and a temperature difference of 20 K (100 observations). The multi-temperature tests were conducted in random order; however, the specimens were not removed from the apparatus between temperature settings.

Except for SRM 1451, the materials were tested at thicknesses determined by each laboratory with the only provision that the clamping pressure exerted on the specimens by the measuring equipment was limited from 1000 Pa to 2000 Pa. For SRM 1451, the test thickness was limited to 25.4 mm by utilizing spacer stops placed at the perimeter of the specimen to prevent over-compression of the material during testing. The use of spacer stops for the other materials (for example, limiting plate movement due to specimen creep, if any) was left to the operator's discretion. The test data were recorded in SI units on "official" data forms and returned to NIST for analysis.

### Fixed Temperature (297.15 K) Replicate Data

Figure 1 plots the measurements of  $\lambda$  (297.15 K) versus laboratory (identified<sup>3</sup> in Table 2) for each of the four materials (Table 1). For each laboratory, the replicate observations are offset along the **x-axis** to assess trends in the run-sequence of an individual laboratory. For laboratories 2, 3, 4, and 5, the data points include symmetric error bars representing the respective laboratory's estimate of expanded uncertainty ( $U$ ) for  $\lambda$  (Table 2). The major conclusions from Figure 1 are as follows:

- 1) For materials 1, 2, and 3, the laboratories differed in average response.
- 2) In contrast, for material 4, the average laboratory responses were essentially the same.
- 3) For materials 1 and 2, laboratory 1 had a significantly high average response.
- 4) For materials 1, 2, and 3, laboratory 2 was consistently higher than laboratory 3.
- 5) For material 3, laboratory 4 was significantly low.
- 6) The differences between the five laboratories changed from material to material – that is, there is a laboratory-material interaction.

---

<sup>3</sup> While planning this study, the laboratory participants decided that the international user communities would derive maximum benefit by open presentation of the data; hence, the data are *not* presented anonymously.

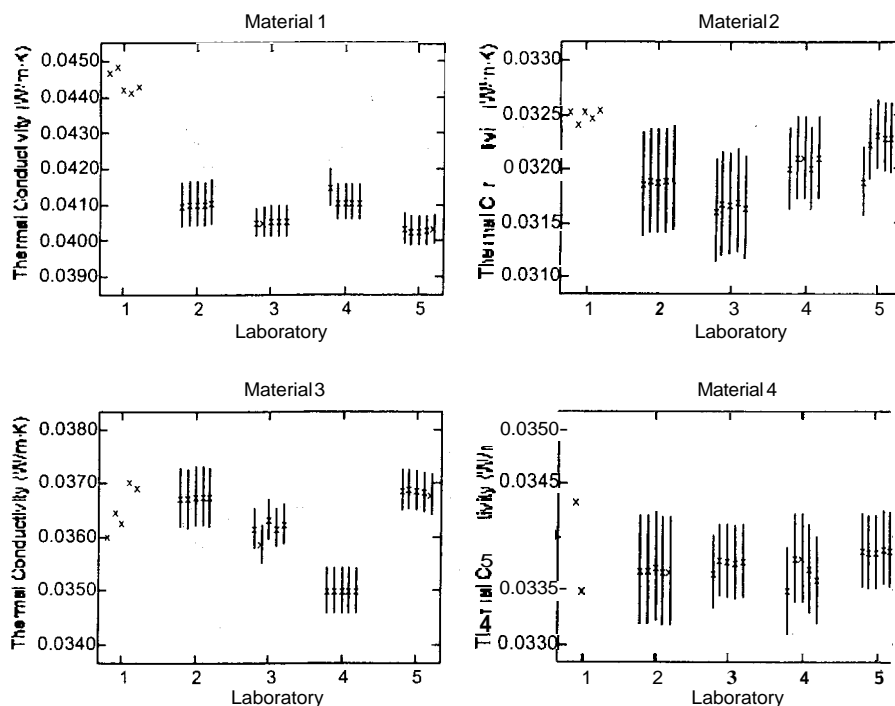


Figure 1 -Replicate data (297.15 K) versus laboratory. Error bars equal laboratory expanded uncertainty (Table 2).

### Summary Statistics

The statistical treatment of interlaboratory data typically involves determining location and variation parameters based on an assumed underlying model for the data. For the fixed temperature (297.15 K) replicate data, there are two primary factors: laboratory (5 levels) and reference material (4 levels). Thus, the underlying model for these data is assumed to have the following form:

$$y = a_{ij} + E \quad (2)$$

where  $y$  is the response variable  $\lambda$ ,  $a_{ij}$  is a constant for laboratory  $i$  and material  $j$ , and  $E$  is error. The effect of temperature as a primary factor, from 280 K to 320 K, is discussed later.

Table 3 summarizes the mean values (location) and standard deviations (variation) for the replicate data (100 observations). Each entry represents the local (5 observations) mean ( $\bar{\lambda}$ ) or standard deviation ( $SD(\lambda)$ ), respectively, for a particular laboratory. The last column provides the respective grand or "pooled" statistic (25 observations) for each

laboratory (across all materials). The last row in each table provides the respective grand or “pooled” statistic (25 observations) for each material (across all laboratories).

Table 3a – Means ~~for~~ Replicates (297.15 K)

	Material 1	Material 2	Material 3	Material 4	Lab
	$\bar{\lambda}$	$\bar{\lambda}$	$\bar{\lambda}$	$\bar{\lambda}$	Average
Lab	(W/m K)	(W/m K)	(W/m K)	(W/m K)	(W/m K)
1	0.04448	0.03251	0.03655	0.03391	0.03686
2	0.04104	0.03189	0.03675	0.03369	0.03584
3	0.04055	0.03166	0.03616	0.03375	0.03553
4	0.04118	0.03206	0.03500	0.03368	0.03548
5	0.04032	0.03220	0.03686	0.03387	0.03581
Average	0.04151	0.03206	0.03626	0.03378	0.03591

Table 3b – Standard Deviations ~~for~~ Replicates (297.15 K)

	Material 1	Material 2	Material 3	Material 4	Pooled
	SD ( $\lambda$ )	SD ( $\lambda$ )	SD ( $\lambda$ )	SD ( $\lambda$ )	SD
Lab	(W/m K)	(W/m K)	(W/m K)	(W/m K)	(W/m K)
1	0.00032	0.00005	0.00043	0.00030	0.00031
2	0.00003	0.00002	0.00002	0.00002	0.00002
3	0.00002	0.00004	0.00017	0.00005	0.00009
4	0.00018	0.00005	0.00000	0.00013	0.00011
5	0.00003	0.00018	0.00004	0.00001	0.00009
Pooled SD	0.00016	0.00009	0.00021	0.00015	0.00016

The last column in Table 3a reveals that the average of laboratory 1 across all four materials is consistently higher than the other laboratories. On the average across all four materials, laboratories 2 and 5, and 3 and 4, are closely paired and each pair of laboratories differs by about 0.8%. The last column in Table 3b reveals that laboratory 1 is consistently noisy across all four materials. Laboratories 3, 4, and 5 exhibit similar levels of variability while laboratory 2 is extremely precise (by nearly a factor of 5 in comparison to the other three laboratories) across all four materials.

### Treatment of Anomalous Data

The results from Figure 1 and Table 3 reveal that the test results for materials 1 and 3 from laboratories 1 and 4, respectively, are significantly different than the other laboratories. In general, the treatment of anomalous (or outlying) data can be handled either by retaining, correcting, or deleting the data. Obviously, none of these options are completely satisfactory; however, the third option (deletion) is acceptable when a physical cause can be identified to explain the behavior of the data. For interlaboratory studies, it is extremely helpful (and inevitably necessary) for the laboratories in question to present their own explanations for the behavior of the test results. To their credit, laboratories 1 and 4 did provide explanations for their anomalous data.

After submission of their test data, laboratory 1 reported that the surface temperatures for determinations of specimen AT were measured using 0.2-mm-diameter

thermocouples placed directly on the surface of the specimen with adhesive tape. In contrast, the other laboratories utilized temperature ~~sensors~~ permanently mounted in the heating and cooling ~~surfaces~~.<sup>4</sup> It is surmised that much of the variability observed in Figure 1 could be attributed to the technique of affixing thermocouples to the specimen surface. **An** early comparison of guarded hot plates [8] noted that discrepancies could result between conductivity values obtained using temperatures ~~from~~ plate surfaces and those measured using surface thermocouples. These data for laboratory 1 and material 1 were considered sufficiently different from the others to warrant rejection as an outlying observation and were omitted in further analyses of the replicate data.

For material 3, laboratory 4 reported values of  $\lambda$  that are 3.5% below the grand mean for material 3. In the comment section of their official test report form, laboratory 4 reported ~~that~~, “this material had completely delaminated on arrival so that the test specimen consisted of two pieces which were always aligned in the same orientation with respect to each other whilst testing.” Unfortunately, although laboratory 4 made a notable effort to test material 3, the ~~specimens~~ received by laboratory 4 were physically different ~~than~~ those received by the other laboratories. Since no other laboratories reported similar experiences, this set of data for material 3 was considered sufficiently different from the other specimens to warrant rejection ~~as~~ an outlying observation and was omitted in ~~further~~ analyses of the replicate data.

### Laboratory-to-Laboratory Differences

Ideally, interlaboratory studies **are** designed to investigate within- and between-laboratory variability of the primary factors by minimizing the effects of secondary laboratory factors. Thus, the resulting variability in the test data may then be attributed to unavoidable random errors present in every experiment. In actuality, however, lab-to-lab differences reflect a confusing mixture of random and systematic errors. **As** noted above, the presence of relatively large lab-to-lab differences offer easier targets for identifying plausible physical explanations. Unfortunately, **as** labto-lab differences approach some minimum level of engineering significance, separating the random and system effects becomes **difficult**, if not impossible. **An** underutilized technique for examining lab-to-lab differences is the cause-and-effect chart.

Figure 2 categorizes 19 secondary factors that could affect the test result of an individual laboratory. The major categories of variation examined in this study include: 1) procedure; 2) specimen; 3) equipment; and, 4) measurement, among others. Here, procedure refers to a particular technique utilized by a laboratory. For example, the technique utilized to determine the AT across the test material. Specimen refers, in this case, to the effect of bulk density ~~within~~ a material. Other material effects, although desirable, were not investigated in **this** study. Equipment covers the component differences noted in Table 2, and measurement covers all properties measured in-situ in

---

<sup>4</sup>Temperature sensors such as thermocouples are typically installed in grooves cut in the surfaces of the plates. For laboratory 3, a platinum resistance thermometer is actually installed in the guard-gap on the perimeter of the meter plate in accordance with ASTM Practice for Guarded-Hot-Plate Design Using Circular Line-Heat Sources practice (C 1043).



the guarded-hot-plate apparatus for the determination of  $\lambda$ . Obviously, this list is not all-inclusive – the effects associated with operator and environment are not considered.

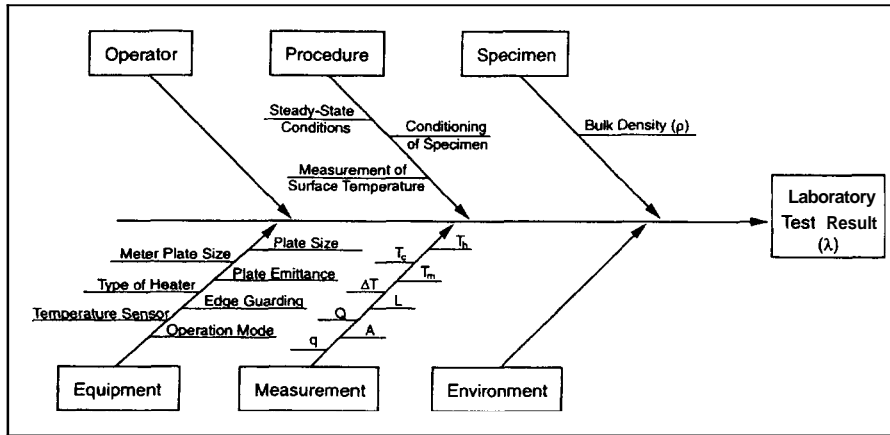


Figure 2 – Cause-and-effect chart for secondary factors.

An analysis of variance (ANOVA) for  $\lambda$  is useful in determining whether there are factor effects on  $\lambda$ . Specifically, values of the ANOVA cumulative probability near 100% are indications of factor significance. Significance, however, does not necessarily imply causation – especially given the fact that many correlations exist among the factors themselves. For example, if  $T_h$  is significant and/or  $T_c$  is significant, then it is not surprising that  $T_m$  and/or  $\Delta T$  would also be significant.

Table 4 summarizes whether a factor is statistically significant. The term *FCDF* (F-cumulative distribution function) is the percent point of the F-distribution [9]; **only** *FCDF* values above 95% are considered significant (i.e., at the 5% level). It is important to note that values of *FCDF* are based on the assumption that the variances of the treatments<sup>5</sup> are constant across treatments – this is decidedly *not* the case for many analyses. An advantage of the ANOVA analysis is that it is applicable to both types of data: quantitative (numeric) or qualitative (categorical).

From Table 4, the single most important conclusion is that, for material 4, the primary factor laboratory is *not* statistically significant. This is not the case for materials 1, 2, and 3 – there is statistically significant difference across the five laboratories. Further examination of Table 4 above indicates that many of the 19 (secondary) laboratory factors are significant. Finding the root significant factor(s) is done by using results from Table 4 in conjunction with engineering judgment (and possibly additional tests) by the participating laboratories.

The nearly homogeneous behavior of the laboratories for material 4 is noteworthy. One possible explanation is material composition. Material 4 is a molded-beads, expanded polystyrene board [6]; the three others are (essentially) fibrous glass and

<sup>5</sup> A treatment is a particular combination of levels of the factors involved in an experiment.

binder, having nominal densities ranging from 13 kg/m<sup>3</sup> to 200 kg/m<sup>3</sup> (Table 1). The cellular nature of polystyrene board, consisting primarily of **small** spheres, would have different anisotropic properties and specimen/plate contact characteristics ~~than~~ the fibrous materials. Another possible explanation is that the relatively ~~thin~~ specimen (13 mm) would have less effect on edge heat losses, if present.

Table 4 – *Is a Factor Statistically Significant? (FCDF > 95 %? Yes/No)*

Laboratory Factors	Material 1	Material 2	Material 3	Material 4
0) Laboratory (primary)	Y	Y	Y	N
1) Steady-state conditions	Y	Y	Y	N
2) Conditioning of specimen	Incomplete	Incomplete	Incomplete	Incomplete
3) Measurement technique for surface temperatures	Y	Y	N	Y
4) Bulk density (p)	Y	Y	Y	N
5) Plate size	Y	Y	N	N
6) Meter plate size	Y	Y	Y	N
7) Plate emittance	Y	Y	Y	N
8) Type of heater	N	Y	N	N
9) Edge guarding	Y	N	Y	N
10) Temperature sensor	N	Y	Y	Y
11) Operation mode	N	N	Y	N
12) T <sub>h</sub>	Y	N	Y	Y
13) T <sub>c</sub>	Y	N	Y	Y
14) T <sub>m</sub>	Y	N	Y	Y
15) AT	Y	Y	Y	Y
16) L	N	Y	Y	N
17) Q	Y	Y	Y	N
18) A	Y	Y	Y	N
19) q	Y	Y	Y	N

### Laboratory Equivalence

Two sets of laboratory data (material 1, laboratory 1 and material 3, laboratory 4) have been identified that **are** sufficiently different to warrant rejection **as** outlying observations based physical causes. Excluding these 10 observations, laboratory **relative** means and the grand **relative** standard deviations **are** re-computed and **summarized** in Table 5.

The laboratory relative standard deviation represents the relative variation of data about the local laboratory **mean**. A low value represents a “tight” or quiet laboratory; correspondingly, a **high** value for the relative *standard* deviation **represents** a “noisy” laboratory. From Table 5, laboratory 2 is **tight** for all four materials. In some cases, **as** noted in Table 5, the laboratory variation is **high** (above 1%) or **marginally** high (approaching 0.5%). With regards to laboratory variation, ISO 8302 specifies a reproducibility<sup>6</sup> limit of **better than** 1% for independent replicate measurements near room temperature. With the exception of one set of **data** (material 3, laboratory 1), the laboratory **standard** deviations **are** all less than 1% (Table 5).

<sup>6</sup> ASTM defines this quantity as repeatability.

Table 5 – *Relative Means and Standard Deviations for Replicates (297.15 K)  
Excluding Outlying Data (Material 1-Lab 1 and Material 3-Lab 4)*

Lab	Material 1		Material 2		Material 3		Material 4	
	Mean (%)	SD (%)	Mean (%)	SD (%)	Mean (%)	SD (%)	Mean (%)	SD (%)
1	----	----	1.4	0.16	–0.1	1.19 <sup>1</sup>	0.39	0.89 <sup>4</sup>
2	0.7	0.07	–0.6	0.06	0.5	0.04	–0.26	0.05
3	–0.5	0.04	–1.3	0.11	–1.1	0.47 <sup>2</sup>	–0.09	0.13
4	1.0	0.43 <sup>2</sup>	0.0	0.17	----	----	–0.30	0.39 <sup>2</sup>
5	–1.1	0.06	0.4	0.56 <sup>1</sup>	0.8	0.11	0.27	0.04
Grand	---	0.91	----	0.95	----	0.95	----	0.49
Range	1.8	----	2.7	----	1.9	----	0.69	----
Half-Range	± 0.9	----	± 1.4	----	± 1.0	----	± 0.35	----

<sup>1</sup>High<sup>2</sup>Marginally high

The laboratory relative mean represents the relative differences of the laboratory mean from consensus values (i.e., the grand mean) for each material. As observed earlier in Figure 1, the differences for many of the laboratories in Table 5 change sign from material to material. It is important to note that the laboratory relative means represent relative differences currently utilized in key comparisons as part of the international Mutual Recognition Agreement [10]. From Table 5, the ranges of laboratory means for materials 1, 2, 3, and 4 are 1.8%, 2.7%, 1.9%, and 0.69%, respectively. The corresponding half-ranges (last row of Table 5) for materials 1, 2, 3, and 4 are ± 0.9%, ± 1.4%, ± 1.0%, and ± 0.35%, respectively.

**Are** the relative differences among laboratories at 297.15 K significant? The answer depends on the uncertainty metric considered, and there **are** several metrics that **can** be used for comparison, including:

- 1) **An** international comparison of a large population (nearly 50) of international guarded-hot-plate laboratories from Africa, Asia, Australia, Europe and North America [11];
- 2) C 177 imprecision statements;
- 3) ISO 8302 uncertainty statements;
- 4) MST SRMs 1451 and 1453 uncertainty limits;
- 5) The **minimum difference** (A) accepted as significant from an engineering perspective;
- 6) Individual laboratory expanded uncertainties as reported in Table 2; and,
- 7) Laboratory statistical significance, ANOVA, 95% as reported in Table 4.

The first metric **is** from a study that was intended to determine the worldwide state-of-the-art in guarded hot plate measurements prior to the development of ISO standards [11]. Participants measured the thermal conductivity of fibrous glass board at mean temperatures of 283 K, 297 K, and a third temperature within the range from 273 K to 313 K. The results indicated that the relative standard deviation of the data from the fitted curve is 2.4%, although several data points deviated from the curve by more than 5% and some by more than 10% [11]. The metrics for 2) to 4) are well **known** and Summarized in Table 6.

The participants have agreed to accept 1.5% as the **minimum** engineering significance difference (**A**) for the above comparison of national standards laboratories. In other words, for national standards laboratories, any difference less than 1.5% from the consensus mean is considered insignificant from an engineering perspective.

Table 6 summarizes the responses (yes **or** no) by material for the seven different uncertainty metrics and their corresponding estimate (in parentheses) at the two standard-deviation level. Note that **only** for material 4 are the laboratories considered equivalent for all the uncertainty metrics. For the other materials, however, the laboratories are considered equivalent with respect to the **minimum** engineering difference of 1.5% (as well **as** the first four uncertainty metrics). For the individual laboratory expanded uncertainty (at  $k = 2$ ) metric, the laboratories **are** not equivalent for materials 1, 2, and 3. Particular combinations of laboratories, however, **are** equivalent **as** shown in Table 6 and these combinations change for materials 1, 2, and 3.

Table 6—*Are the Laboratories Equivalent at 297.15 K? (Yes/No)*

Uncertainty Metrics (2 $\times$ Standard Deviation)	Material 1 ( $\pm 0.9\%$ )	Material 2 ( $\pm 1.4\%$ )	Material 3 ( $\pm 1.0\%$ )	Material 4 ( $\pm 0.35\%$ )
1) International <i>GHP</i> Study (4.8%) [11]	Y	Y	Y	Y
2) ASTM C 177 (2% to 5%)	Y	Y	Y	Y
3) ISO 8302 (2% to 5%)	Y	Y	Y	Y
4) SRMs 1451 (3%) and 1453 (1.3%)	Y	---	---	Y
5) <b>Minimum Engineering Significance <math>\Delta</math> (1.5%)</b>	Y	Y	Y	Y
6) Laboratory Uncertainty (1.0% to 1.5%)	N:(2,4)(3,5)	N:(2,3)(4,5)	N:(1,2,5)(3)	Y
7) Statistical Significance ( <b>ANOVA</b> , 95%)	N	N	N	Y

#### Multi-Temperature Data (280 K to 320 K)

For the multi-temperature data, there are three **primary** factors: laboratory (5 levels), reference material (**4** levels), and temperature (5 levels). Although the single data-point **at** each temperature precludes a rigorous statistical analysis, the analyses are driven by the same central theme considered for the fixed-temperature replicate data: **How** do the laboratories behave across the four materials? In particular, what **are** the location and variation estimates for each material? Examination of **these** questions is provided by a **linear** regression **analysis** of the multi-temperature data using the following model:

$$A = b_0 + b_1 T_m \quad (3)$$

where  $\hat{\lambda}$  is the predicted value for Eq 3 based on least-squares estimates for  $b_0$  and  $b_1$ .

Figure 3 plots the relative deviations from the fitted curve for each data point. **As** observed with the replicate **data**, the principal conclusion from Figure 3 is that the behavior of the laboratories does, in fact, change from material to material. For the four plots, the location and variation of each set of laboratory data changes from material to material. Further examination of the slopes reveals that there **is a** change in slope for several laboratories (most notably for laboratories 1, 2, and 5). A final conclusion of Figure 3 is that the relative deviations among the laboratories **are** affected substantially **as**

the mean temperature decreases from room-temperature conditions. This conclusion is less evident if data from laboratory 1 are omitted.

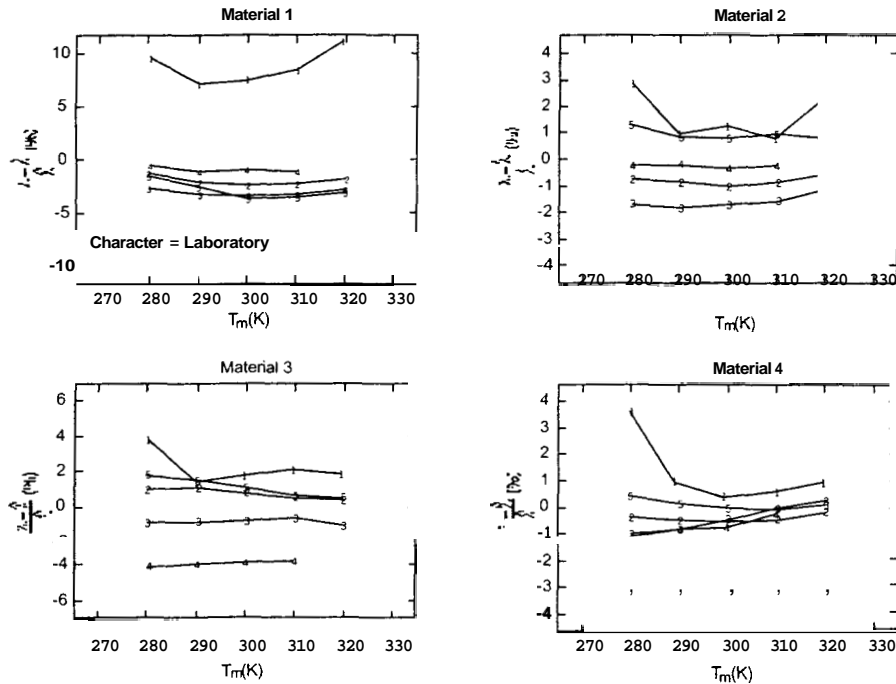


Figure 3 – Multi-plot of relative deviations versus mean temperature.

### Conclusions

This international comparison investigated the variability in thermal conductivity results among guarded hot plate laboratories in Canada, France, Japan, the United Kingdom, and the United States using four regional/national reference materials. The reference materials were SRM 1451 (fibrous-glass blanket), IRMM-440 (resin-bonded glass fibre board), JTCCM “candidate” mineral-oxide fiberboard, and SRM 1453 (expanded polystyrene board). The collaboration assessed the effects of two primary factors – laboratory and material – for five replicate measurements at 297.15 K (24 °C), and included a third primary factor – temperature – for single-point measurements at 280 K, 290 K, 300 K, 310 K, and 320 K.

The thermal conductivity test data (Figures 1 and 3) indicate that there is a laboratory-to-laboratory difference for each of the materials, except SRM 1453. As expected, there is a material-to-material difference – material 1 (SRM 1451) was the highest thermal conductivity; material 2 (IRMM-440) was the lowest. This material-to-material difference was greater than the laboratory-to-laboratory difference. Ranking the

materials by variability (all data included) yields the following order (lowest to highest): material 4 (SRM 1453), material 2 (IRMM-440); material 3 (JTCCM “candidate”); and, material 1 (SRM 1451). The results of the multi-temperature (280 K to 320 K) data were consistent with the results observed for the fixed-temperature (297.15 K) replicate data. In addition, the results indicated that disagreement among the laboratories tended to increase as mean temperatures decreases from 297.15 K.

Two of the replicate data sets (at 297.15 K) were identified as anomalous and later excluded after the laboratories in question identified physical causes for the behavior of their data. After exclusion of the anomalous data, the half ranges for materials 1, 2, 3, and 4 were  $\pm 0.9\%$ ,  $\pm 1.4\%$ ,  $\pm 1.0\%$ , and  $\pm 0.35\%$ , respectively. These laboratory-to-laboratory differences are considered small by many different uncertainty metrics, including ISO 8302 uncertainty statements, C 177 precision indices, and NIST SRM uncertainty statements, among others. For this comparison, the laboratory participants have accepted a minimum engineering significance difference of 1.5% from the consensus mean for national standards laboratories. In other words, laboratory differences less than 1.5% from the consensus mean are currently considered insignificant based on an engineering perspective.

One of the most plausible factors affecting the test data was procedural in nature. In particular, a significant difference in average value and variation was experienced by one laboratory that affixed temperature sensors directly to the specimen surface rather than using permanent sensors affixed to the apparatus plates. The approach of adhering fine-diameter temperature sensors to the specimen surface appears to have contributed to measurement differences and may be an *unintended* extension of the test procedures specified in ISO 8302 and C 177. Further measurements comparing different techniques for determining the temperature difference across a test specimen would be extremely useful. With regard to ISO 8302 and C 177, the appropriate sections on determination of the temperature difference should be reexamined for clarity and revised, if necessary.

### Acknowledgments

The authors appreciate the cooperation, openness, professionalism, and hard work of the following individuals and laboratories: Masayoshi Uezono (JTCCM), Gianni Venuti (LNE), David Salmon (NPL), Ronald Tye (NPL), Kumar Kumaran (NRCC), and Fitsum Tariku (NRCC). The authors appreciate the donation of one material (IRMM-440) by the European Commission Institute for Reference Materials and Measurements through the efforts of Jean Pauwels, Andrée Lamberty, and Chris Ingelbrecht. We gratefully acknowledge the efforts of Eric Lagergren, who developed the test plan utilized in this collaboration.

### References

- [1] McCaa, D. J., “Standard Reference Materials: C 518 Heat Flow Meter,” *Standard Reference Materials: Issues and Concerns for the Future, ASTM C-16 Workshop*, New Orleans, LA, 1996.

- [2] Zarr, R. R. and Filliben, J. J., "International Comparison of Guarded **Hot Plate Apparatus** Using National and Regional Reference Materials," *NIST Technical Note 1444*, U.S. Government **Printing** Office, Washmgton D.C., 2002.
- [3] Zarr, R. R. and Filliben, J. J., "Collaborative Thermal Conductivity Measurements of Fibrous Glass and Expanded Polystyrene Reference Materials," *Proceedings of the 26th ITCC/14th ITES Conferences, 2001* (in publication).
- [4] Hust, J. G., "Standard Reference Materials: Glass Fiberblanket SRM for Thermal Resistance," *NBS Special Publication, 260-103* U.S. Government Printing Office, Washington D.C., 1985.
- [5] Quin, S. Venuti, G., DePonte, F., and Lamberty **A.**, "Certification of a Resin-Bonded Glass Fibre Board for Thermal Conductivity between  $-10^{\circ}\text{C}$  and  $+50^{\circ}\text{C}$ : IRMM-440," *EUR 19572 EN*, 2000.
- [6] Zarr, R. R., Davis, M. W., and Anderson, E. H., "Room-Temperature Thermal Conductivity of Expanded Polystyrene Board for a Standard Reference Material," *NISTIR 5838*, 1996.
- [7] ISO, "Guide to the Expression of Uncertainty in Measurement," ISBN 92-67-10188-9, 1st Edition, *ISO*, Geneva, Switzerland, 1993; see also Taylor, B. N. and Kuyatt, C. E., "Guidelines for Evaluating and Expressing the Uncertainty of MST Measurement Results," *NIST Technical Note 1297*, U.S. Government Printing Office, Washington D.C., 1994; available at <http://physics.nist.gov/Pubs/>.
- [8] Robinson **H. E.** and Watson, T. W., "Interlaboratory Comparison of Thermal Conductivity Determinations With Guarded Hot Plates," *ASTM STP 119*, 1951, pp. 36-44.
- [9] Snedecor, G. W. and Cochran, W. G., *Statistical Methods*, 6<sup>th</sup> Edition, Iowa State University Press, Ames, Iowa, USA, 1967, **p.** 117.
- [10] Mutual Recognition Arrangement (MRA): JCRB and BIPM Key Comparison Database, URL: [http://h14.bipm.fr/enus/8\\_Kcv\\_Comparisons/introduction.html](http://h14.bipm.fr/enus/8_Kcv_Comparisons/introduction.html), Bureau International des Poids et Mesures, Sevres, France, 28 February 2001.
- [11] **Smith**, D. R. "Thermal Conductivity of Fibrous Glass Board by Guarded Hot Plates and Heat Flow Meters: An International Round-Robin," *International Journal of Thermophysics*, Vol. 18, 1997, pp. 1557-1573